Certificate of analysis

ARA-290 10mg · purity 99.56%

Laboratory

Name	Cupel
Address	2599 Speakman Dr Mississauga, ON L5K 1B1
Web	cupel.ca
Email	help@cupel.ca

Report

Report number	CL-59J7-C5WZ-R
Status	Issued
Issue date	2 October 2026

Sample

Product as labelled	ARA-290 10mg
Submitted by	Lux Peptides
Sender's lot	LP-7899
Appearance	White Lyophilized Powder
Received	23 September 2026
Reported	2 October 2026



Results

Test	Result	Notes
Identity (LC-MS)	**ARA-290**	–
Purity (HPLC-UV)	**99.56%**	–
Net Content	**9.66 mg**	–
Endotoxin Replicate 1	**Pass**	Assay Sensitivity: <=0.05 EU/mL
Endotoxin Replicate 2	**Pass**	Assay Sensitivity: <=0.05 EU/mL

Methods

Endotoxin testing performed using Limulus Amebocyte Lysate assay in accordance with USP <85>.

Analysed by

Timothy Ian Benedicto

Timothy Ian Benedicto
Medical Laboratory Technician

Reviewed and released by

Roxanne Manlapaz

Roxanne Manlapaz
Laboratory Technician


Verify

cupel.ca/verify · CL-59J7-C5WZ-R

SHA-256 of the report data (record.json, served at cupel.ca/r/CL-59J7-C5WZ-R/)

ed7dc4e0ad1cbf929048d2dd476762a8ebd48e98d1ae362899cd20a2db51a1eb

Chromatogram

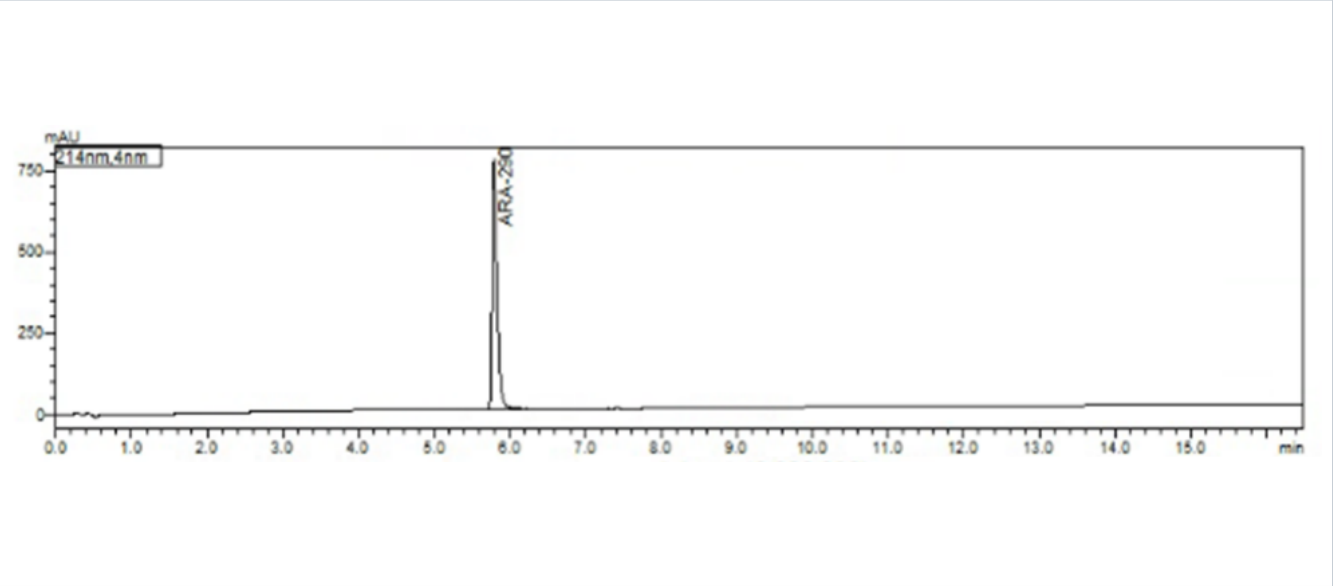

Mass spectrum

