Certificate of analysis

Bacteriostatic Water (BAC) 10ML · purity 99.86%

Laboratory

Name	Cupel
Address	2599 Speakman Dr Mississauga, ON L5K 1B1
Web	cupel.ca
Email	help@cupel.ca

Report

Report number	CL-36TB-X9EZ-5
Status	Issued
Issue date	6 October 2026

Sample

Product as labelled	Bacteriostatic Water (BAC) 10ML
Submitted by	Lux Peptides
Sender's lot	LP-8473
Appearance	Clear Liquid
Received	25 September 2026
Reported	6 October 2026



Results

Test	Result	Notes
Identity (LC-MS)	**Benzyl Alcohol**	–
Purity (HPLC-UV)	**99.86%**	–
Net Content	**0.94%**	–
Endotoxin Replicate 1	**Pass**	Assay Sensitivity: <=0.05 EU/mL
Endotoxin Replicate 2	**Pass**	Assay Sensitivity: <=0.05 EU/mL

Methods

Endotoxin testing performed using Limulus Amebocyte Lysate assay in accordance with USP <85>.

Analysed by

Timothy Ian Benedicto

Timothy Ian Benedicto
Medical Laboratory Technician

Reviewed and released by

Roxanne Manlapaz

Roxanne Manlapaz
Laboratory Technician


Verify

cupel.ca/verify · CL-36TB-X9EZ-5

SHA-256 of the report data (record.json, served at cupel.ca/r/CL-36TB-X9EZ-5/)

94fcc9e94a60667d848150f3d446081fa9ae7fa6a1519032f5a1e7059e0f5d97

Chromatogram

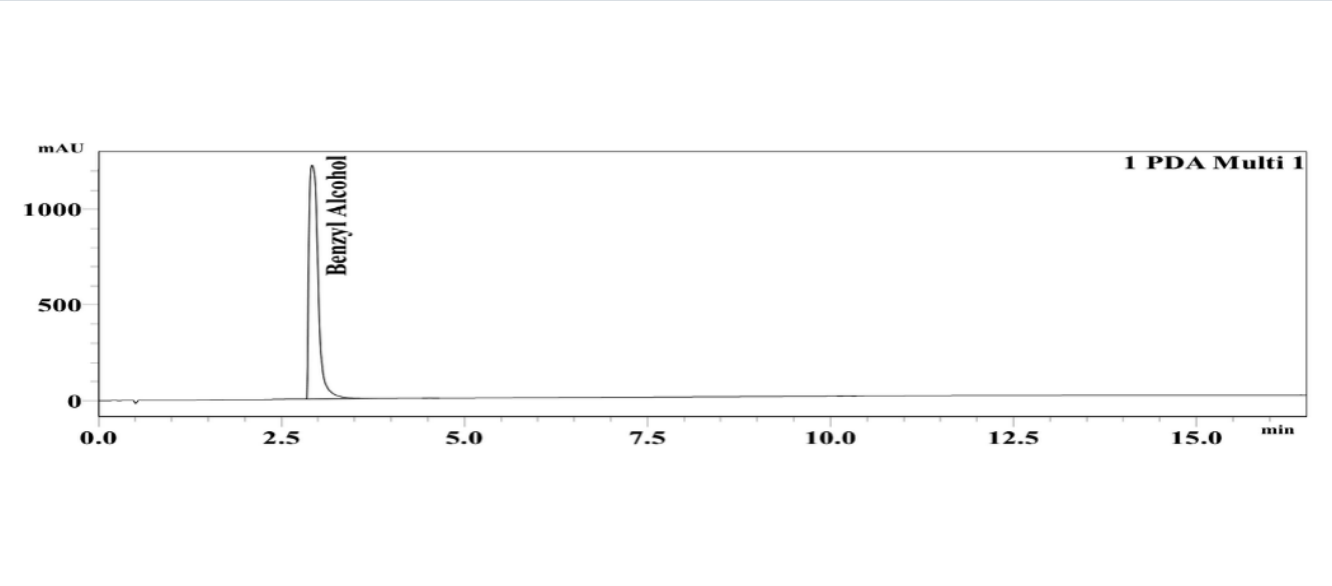

Mass spectrum

