Certificate of analysis

DSIP 10mg · purity 99.11%

Laboratory

Name	Cupel
Address	2599 Speakman Dr Mississauga, ON L5K 1B1
Web	cupel.ca
Email	help@cupel.ca

Report

Report number	CL-XSSZ-M9M8-E
Status	Issued
Issue date	24 September 2026

Sample

Product as labelled	DSIP 10mg
Submitted by	Lux Peptides
Sender's lot	LP-9171
Appearance	White Lyophilized Powder
Received	17 September 2026
Reported	24 September 2026



Results

Test	Result	Notes
Identity (LC-MS)	**DSIP**	–
Purity (HPLC-UV)	**99.11%**	–
Net Content	**11.64 mg**	–
Endotoxin Replicate 1	**Pass**	Assay Sensitivity: <=0.05 EU/mL
Endotoxin Replicate 2	**Pass**	Assay Sensitivity: <=0.05 EU/mL

Methods

Endotoxin testing performed using Limulus Amebocyte Lysate assay in accordance with USP <85>.

Analysed by

Timothy Ian Benedicto

Timothy Ian Benedicto
Medical Laboratory Technician

Reviewed and released by

Roxanne Manlapaz

Roxanne Manlapaz
Laboratory Technician


Verify

cupel.ca/verify · CL-XSSZ-M9M8-E

SHA-256 of the report data (record.json, served at cupel.ca/r/CL-XSSZ-M9M8-E/)

f00cd696afd45befb9888bf88482d0e60ab72149eba22071dfed596aebf9fea1

Chromatogram

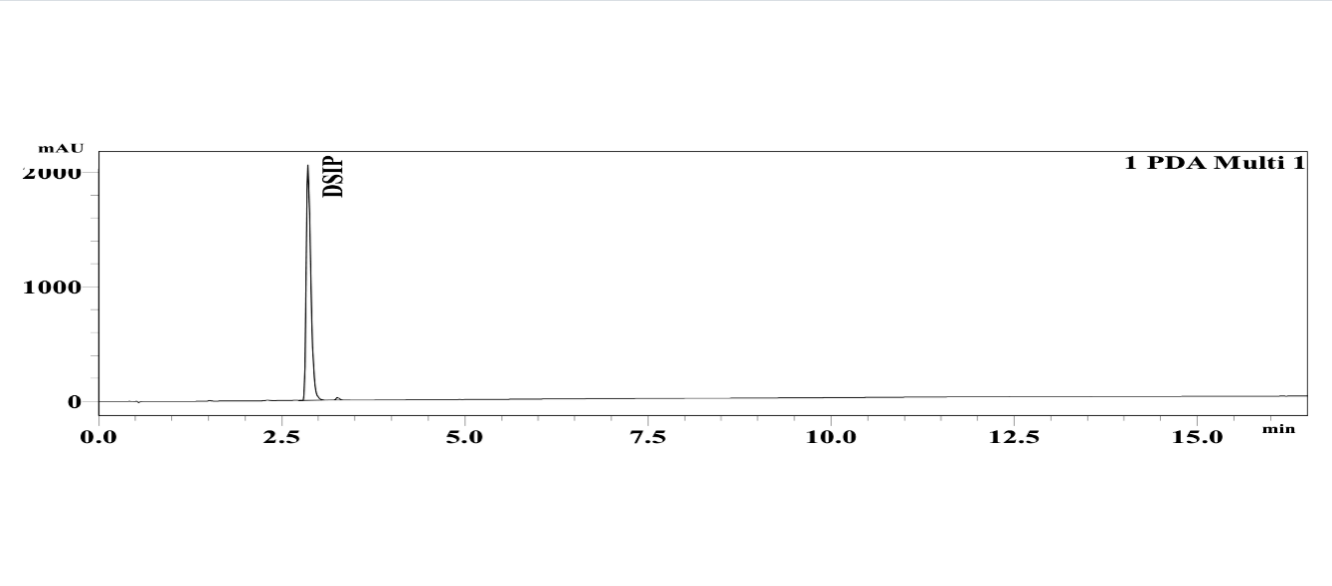

Mass spectrum

