Certificate of analysis

SS-31 50mg · purity 99.74%

Laboratory

Name	Cupel
Address	2599 Speakman Dr Mississauga, ON L5K 1B1
Web	cupel.ca
Email	help@cupel.ca

Report

Report number	CL-E744-NXZN-Y
Status	Issued
Issue date	7 October 2026

Sample

Product as labelled	SS-31 50mg
Submitted by	Lux Peptides
Sender's lot	LP-8959
Appearance	White Lyophilized Powder
Received	28 September 2026
Reported	7 October 2026



Results

Test	Result	Notes
Identity (LC-MS)	**Confirmed**	–
Purity (HPLC-UV)	**99.74%**	–
Net Content	**53.25 mg**	–
Endotoxin Replicate 1	**Pass**	Assay Sensitivity: <=0.05 EU/mL
Endotoxin Replicate 2	**Pass**	Assay Sensitivity: <=0.05 EU/mL

Methods

Endotoxin testing performed using Limulus Amebocyte Lysate assay in accordance with USP <85>.

Analysed by

Timothy Ian Benedicto

Timothy Ian Benedicto
Medical Laboratory Technician

Reviewed and released by

Roxanne Manlapaz

Roxanne Manlapaz
Laboratory Technician


Verify

cupel.ca/verify · CL-E744-NXZN-Y

SHA-256 of the report data (record.json, served at cupel.ca/r/CL-E744-NXZN-Y/)

4eccc2e06af0b345870b896260885dda8e760035ebe67e5f74f1d6be68b1e823

Chromatogram

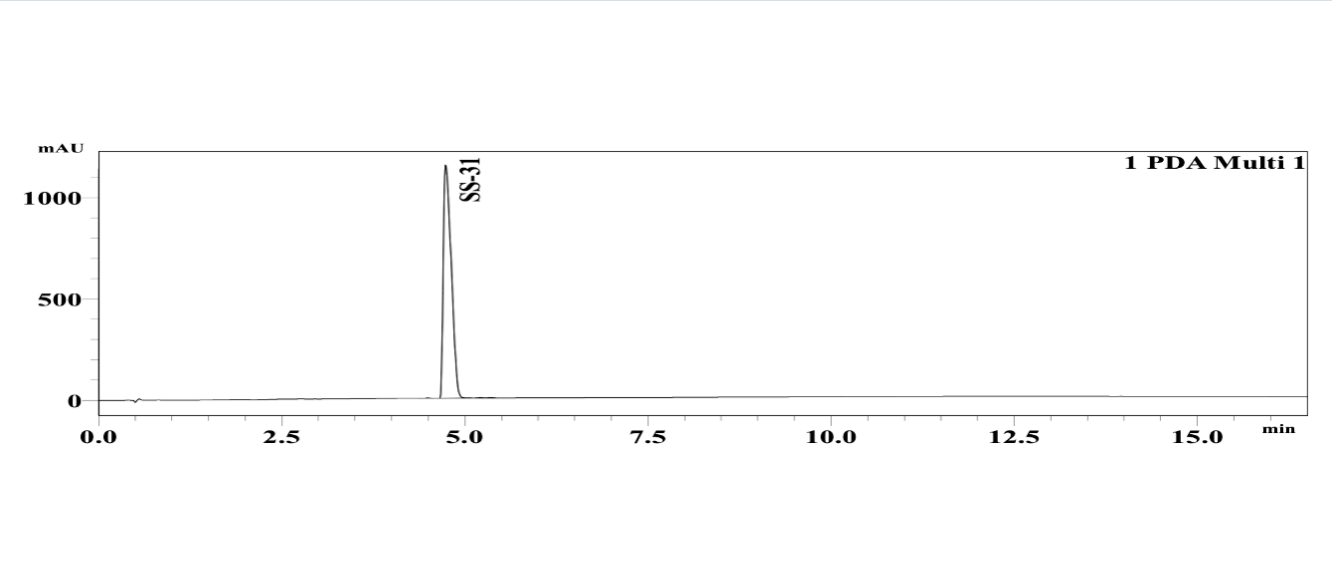

Mass spectrum

